

The Design of Ventilator Algorithm

Chunyan Meng

Center of Computer, Taiyuan Normal University
Taiyuan 030012, China
lvshuyang@163.com

Abstract: This paper designed one ventilator arithmetic. The system is available to various ventilation modes, depending on the on-off state of the proportional valve and the motor. The whole design dealt with the ventilation mode algorithm and the PID control algorithm in different layers.

The ventilator for therapy is for the severely sick and asks for the ability to realize a variety of ventilations depending on the needs[1]. The algorithm of ventilator directly determines the ventilation modes and performance, so reliable ventilator algorithm design is the key technology. It is a guarantee to the performance of ventilator algorithm to configurate and simulate the software and the hardware of the ventilator flexibly when the LabVIEW based ventilator control system is at the prototype developing stage[2].

Key words: Ventilator Arithmetic; PID control; Ventilator

1. the LabVIEW based ventilator control system

The system is available to various ventilation modes, depending on the on-off state of the proportional valve and the motor. The proportional valve, the motor with its driving circuit, and the sensor with its amplifying circuit in the system are practical physical devices, while the human-computer interface, the ventilation mode algorithm and the PID controller are fulfilled by running a LabVIEW program on two computers. The upper computer with the Window XP Operating System achieves the human-computer interface and the ventilation mode algorithm, and the lower Desktop PC with the NI Data Acquisition Card and the LabVIEW RT module achieves data acquisition and PID control.

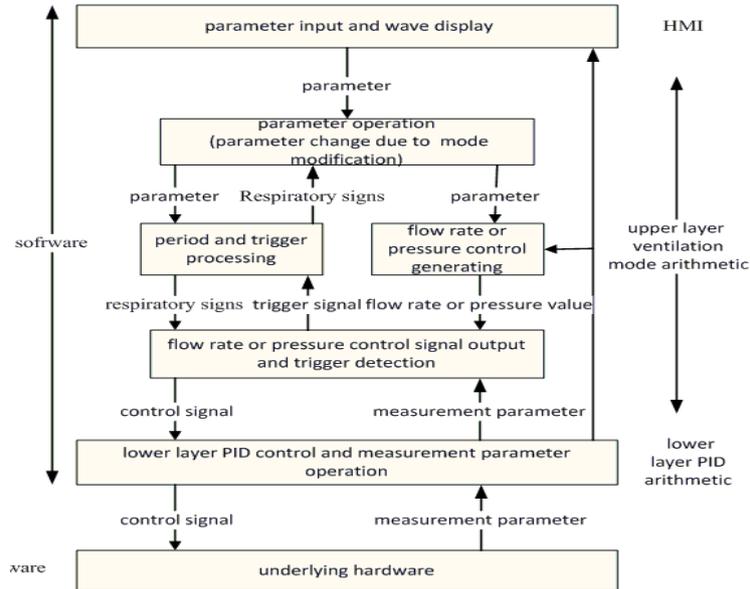


Fig.1 Algorithm structure chart

2. Algorithm structure

The ventilation algorithm design has a double-layer structure, as shown in Fig.1. The upper layer is the ventilation mode algorithm, while the lower layer is the PID control algorithm. The lower layer serves the upper layer and to achieve the constant voltage or current control the upper layer required. It is a Nested structure control algorithm in time sequence structure, as shown in Fig.2. The ventilation mode algorithm and the PID control algorithm work at different periods. The former has a ventilation period R , characterized by seconds. The latter has a practical flow rate and pressure control sampling period T , characterized by milliseconds. The period R is three orders larger than the period T . The upper layer determines the functionality of the ventilator, while the lower layer determines the performance of the ventilator.

3. Lower layer PID controller design

The PID controller of the ventilator adopts the constant current PID controller or the constant voltage PID controller, depending on different ventilation modes and ventilation stages. The best proportional, integral and differential coefficient of different flow rates or pressures are determined by different constant current or constant voltage levels, i.e. the sectional PID controller, through experimental methods. The PID control uses incremental PID control algorithm, and limits the value of increment and output [4,5]. The algorithm is as follows:

The Design of Ventilator Algorithm

$\Delta u(k) = K_p * \Delta e(k) + K_i * e(k) + K_d * [\Delta e(k) - \Delta e(k-1)]$, where $\Delta e(k) = e(k) - e(k-1)$.

If $\Delta u(k) >$ upper range value, then $\Delta u(k) =$ upper range value;

If $\Delta u(k) <$ lower range value, then $\Delta u(k) =$ lower range value.

$u(k) = u(k-1) + \Delta u(k)$, where $u(k)$ is the K th sampling value of the controller's output.

If $u(k) >$ upper range value, then $u(k) =$ upper range value;

If $u(k) <$ lower range value, then $u(k) =$ lower range value.

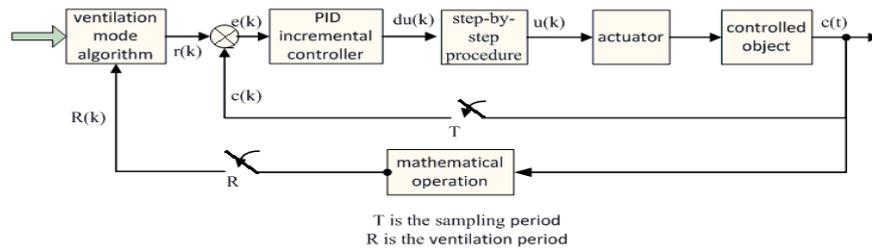


Fig.2 Algorithm structure chart

Where K_p , K_i , K_d are proportional, integral and differential coefficient, respectively, and they are determined by the ventilation flow rate or the pressure level. $e(k)$ is the difference between the designed value and the output value at the moment of K . The output of the PID controller controls the proportional valve and the motor directly, stabilizing the ventilation flow rate and the pressure at a given value.

4. Upper layer ventilation mode design

The ventilation mode algorithm is carefully designed through building block design. There are five ventilation modes, comprising VCV, BiLevel, PRVC, SIMV and CPAP. Each ventilation mode is individually designed and comprises four modules, as shown in Fig.1, which are the parameter operation module, the period and trigger processing module, the flow rate or pressure control generating module and the flow rate or pressure control signal output and trigger detection module.

The period and trigger processing module is the core of each mode algorithm, which generates ventilation time sequence, deals with errors such as trigger and pressure excess, and creates respiratory signs to control the rhythm of the other three modules. The design rules are:

1. Take expiration as the start of each ventilation period;
2. Take each period as the time tick, and each time tick accomplishes the tasks within it;
3. Each time tick comprises of the available trigger state and the ventilation state, and the tasks are mutually exclusive and accomplished individually at each time area. In other words, only one task is dealt at one time point;

The parameter operation module controls user defined ventilation parameters at human-computer interface, such as the operation time of the ventilation mode and tidal volume, in order to avoid abrupt changes due to parameter modification when

ventilation is in progress and to guarantee the accomplishment of the current tasks at the current period.

The flow rate or pressure control generating module converts user defined ventilation parameters at human-computer interface, such as ventilation frequency and tidal volume, to corresponding flow rate or pressure value. It receives the sampling value of sensors to modify flow rate or pressure control value at the same time, in order to accomplish feedback control, as shown in Fig.2. PRVC is the typical application of the feedback control.

The flow rate or pressure control signal output and trigger detection module converts the flow rate or pressure value, which the flow rate or pressure control generating module generates, to the flow rate or pressure control signal according to the respiratory signs, which period and trigger processing module generates. It is applied to the lower layer PID controller and detects the trigger which the patient's active expiration generates. The flow rate or pressure control signal generates and triggers detections under close supervision of the respiratory signs, and the control signal or trigger detections are generated only if the corresponding respiratory signs is valid.

The ventilation mode algorithm program is shown in Fig.3. The program could do Hardware-in-Loop Simulation when embedded in the LabVIEW based ventilator control system.

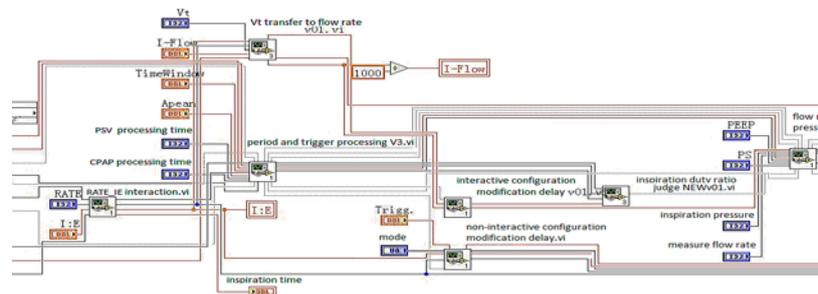


Fig.3 the ventilation mode algorithm program

5. Conclusion

This paper focused on the design of the ventilator algorithm and Hardware-in-Loop Simulation on the LabVIEW based ventilator control system. The Hardware-in-Loop Simulation on the LabVIEW based ventilator control system corrected the algorithm error timely, optimized the performance of the algorithm and met the design specification perfectly.

Reference

- 1 Wang Baoguo. Clinical Application of Ventilators, Beijing: PEOPLE'S MEDICAL PRESS, 2005: 108-130
- 2 Tang Min etc. Based on the LabVIEW platform for rapid construction of medical

The Design of Ventilator Algorithm

- electronic equipment prototype EDN Design of electronic technology
2008.07:138-140
- 3 National Instruments LabVIEW v8.6 Real Time Module user Manual 2008
 - 4 Tao Yonghua etc. The new PID control and its application Beijing : CHINA
MACHINE PRESS , 2001: 1-27
 - 5 Liu Jinkun Advanced PID control MATLAB simulation (Second Edition) Beijing
: PUBLISHING HOUSE OF ELECTRONICS INDUSTRY , 2007: 10-90